



**2013-2014 Wet Weather WQO Ratios
for S28 Dominguez Channel at Artesia Blvd.**

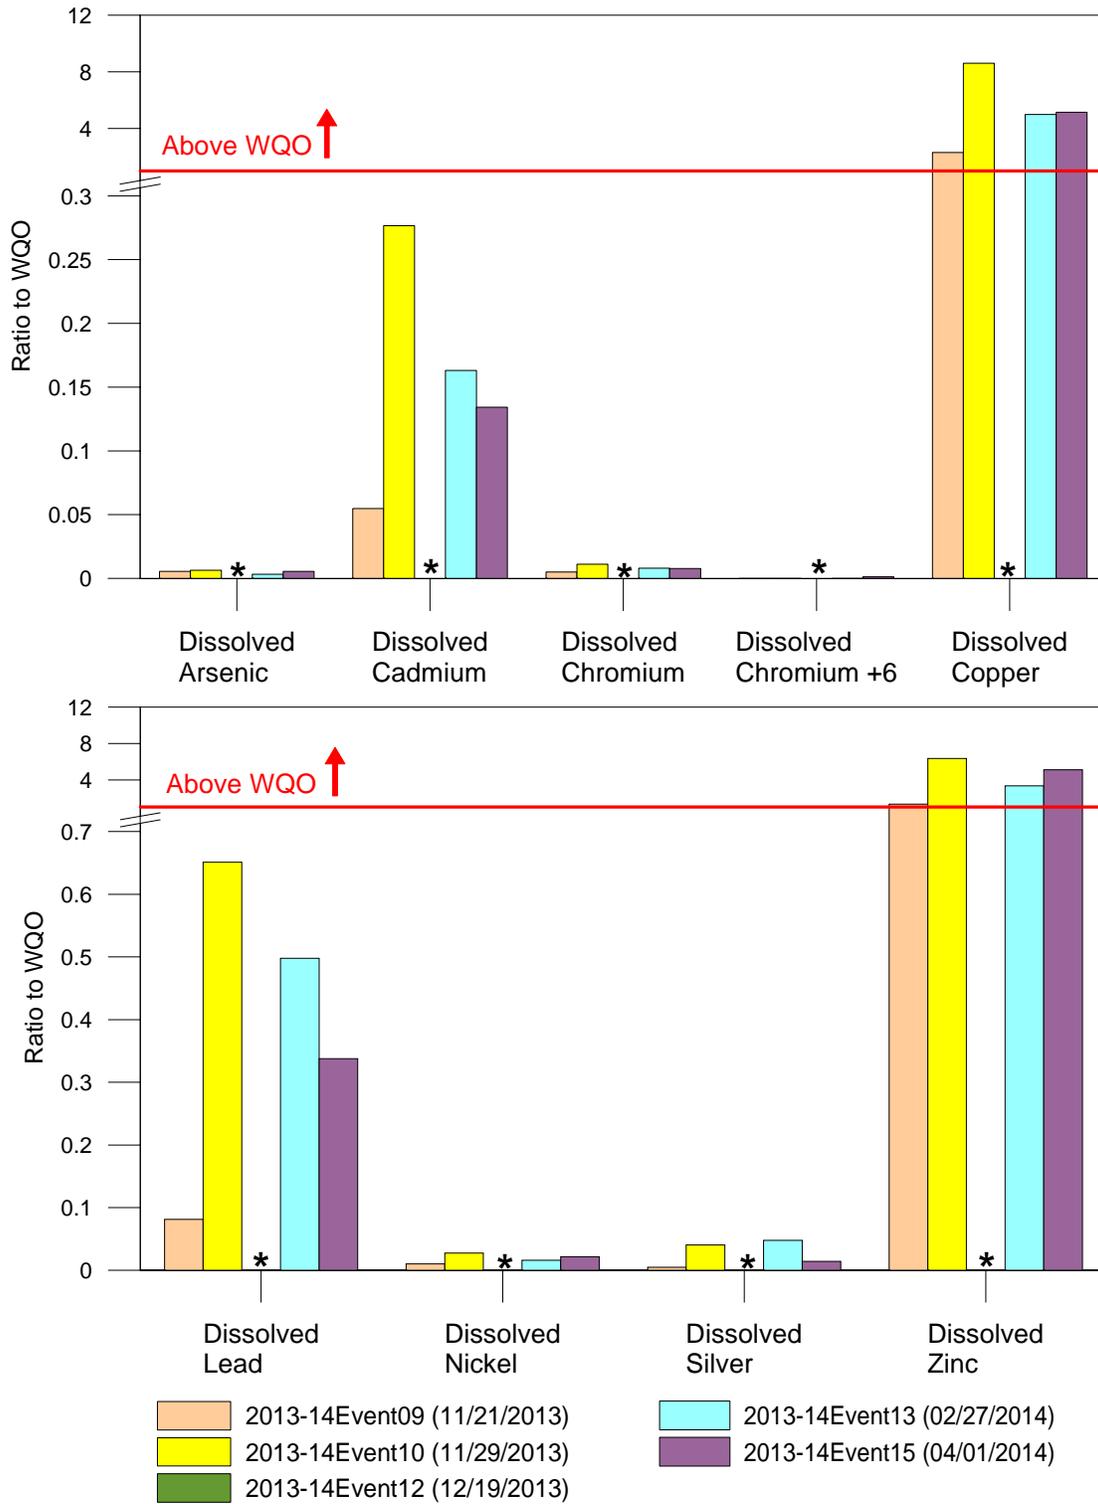

*Samples were not collected for dissolved metals during Event 12.

Figure 4-3.6 S28 Dominguez Channel at Artesia Blvd Wet Weather Ratio Plots


**2013-2014 Wet Weather WQO Ratios
for S28 Dominguez Channel at Artesia Blvd.**

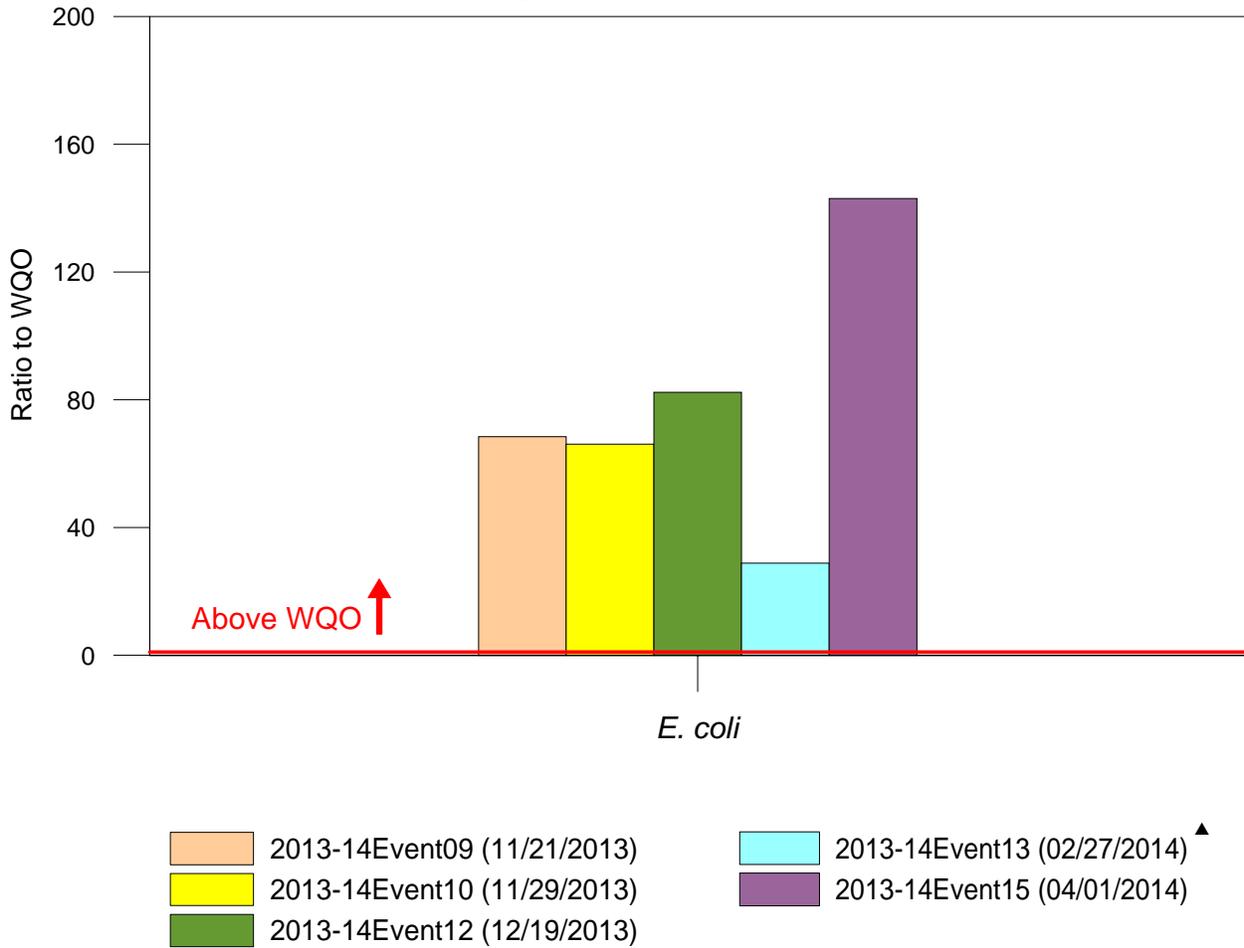

▲Not an exceedance of the E. coli water quality objective due to the High Flow Suspension of Recreational Uses (LARWQCB, 2003).

Figure 4-3.6 S28 Dominguez Channel at Artesia Blvd Wet Weather Ratio Plots

**2013-2014 Wet Weather WQO Ratios
for S28 Dominguez Channel at Artesia Blvd.**

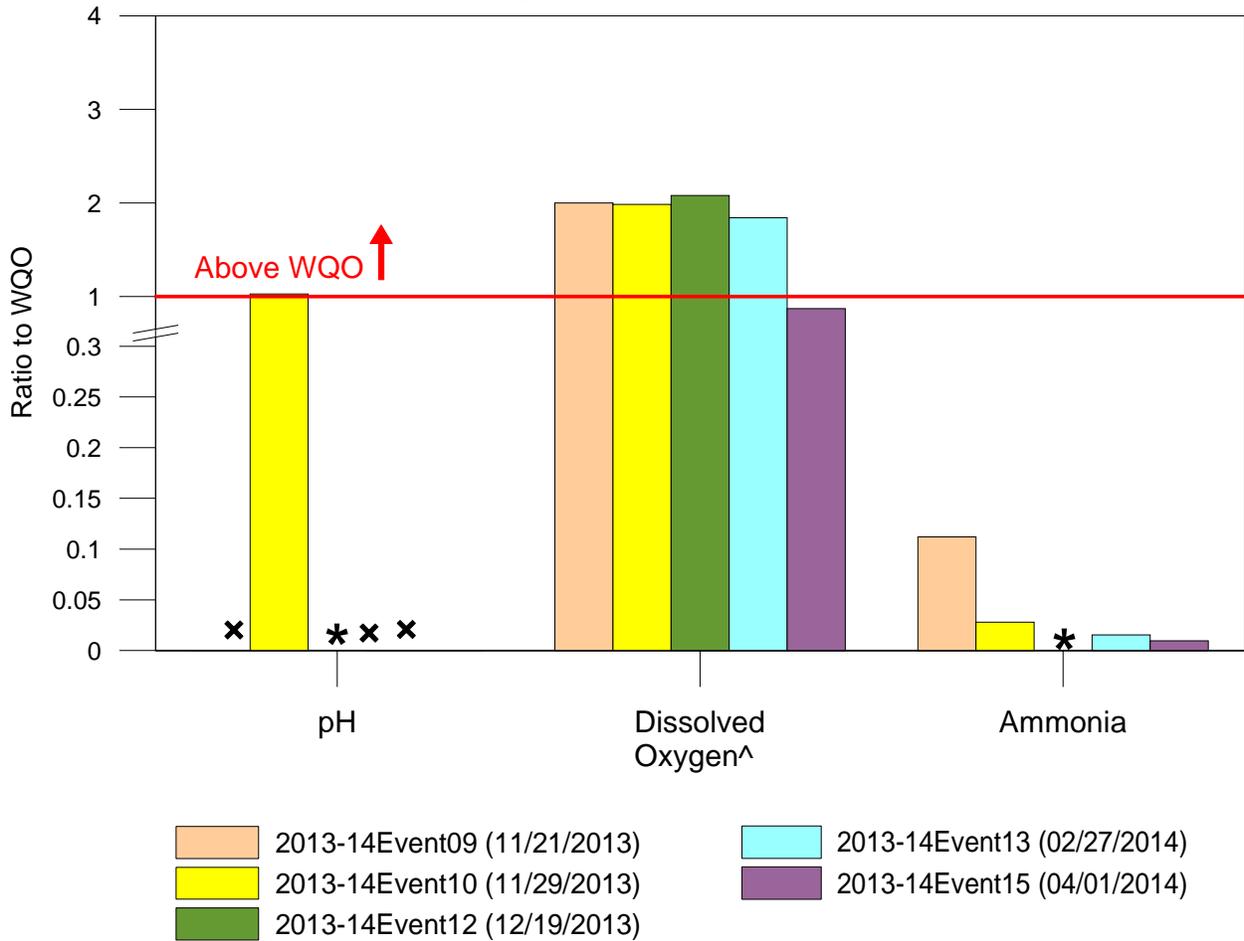

[^]Dissolved oxygen is an exceedance if ratio to WQO is below 1.

x pH was within WQO range.

*Samples were not collected for ammonia or pH during Event 12.

Figure 4-3.6 S28 Dominguez Channel at Artesia Blvd Wet Weather Ratio Plots